

Fig. 1

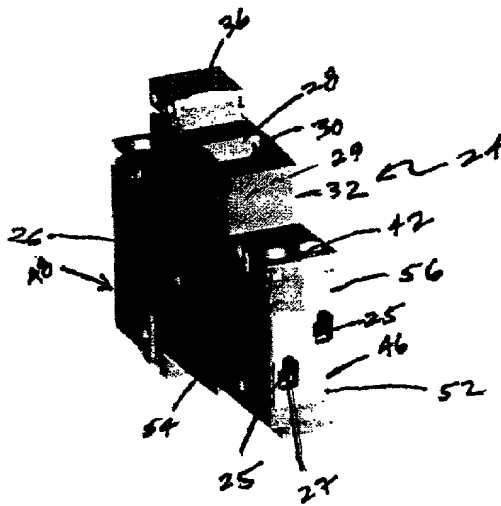


Fig. 2

FIG. 3 is a cross-sectional view of the device taken along line 3-3 of FIG. 1.

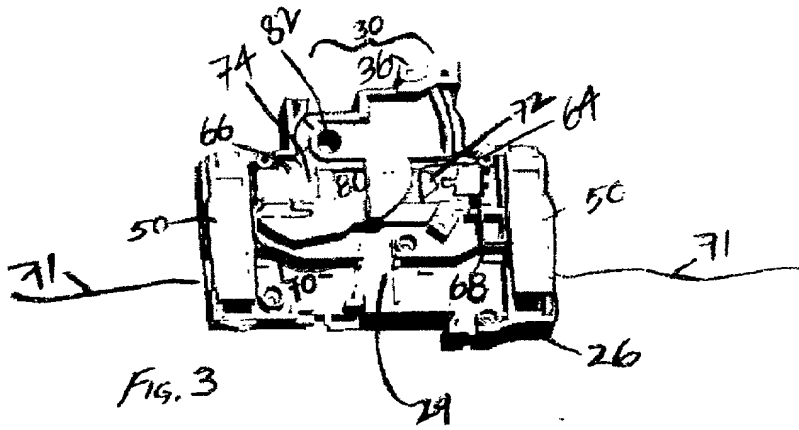


FIG. 3

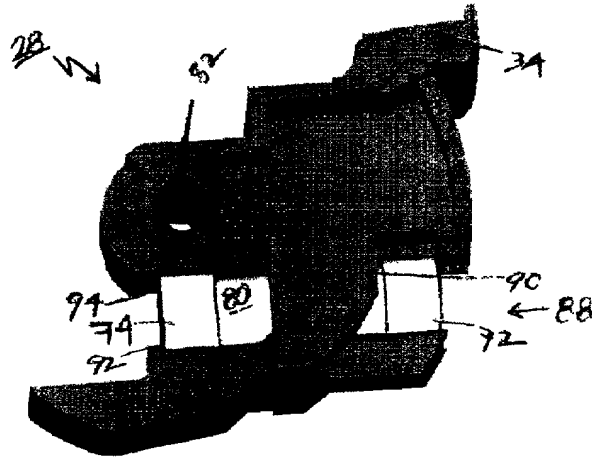


FIG. 4



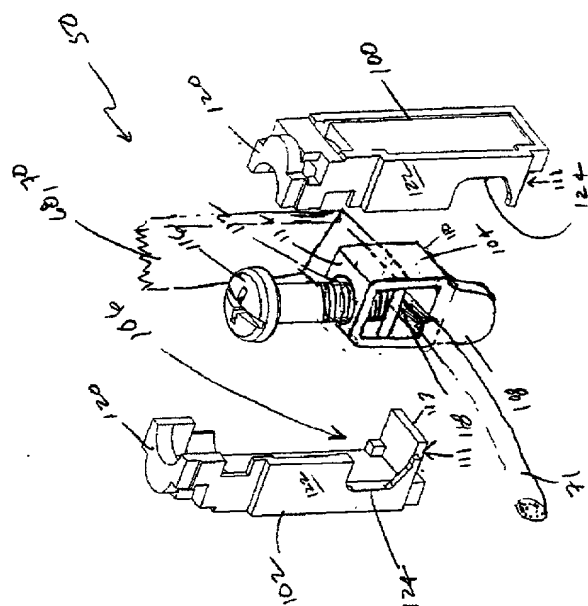


Fig. 6

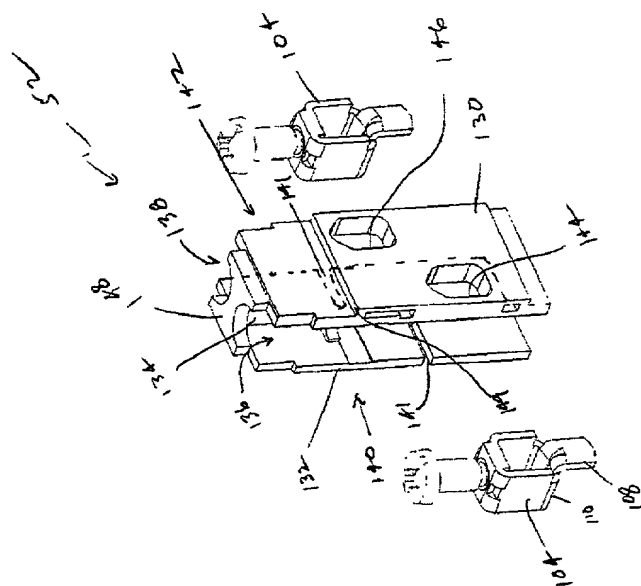


Fig. 7

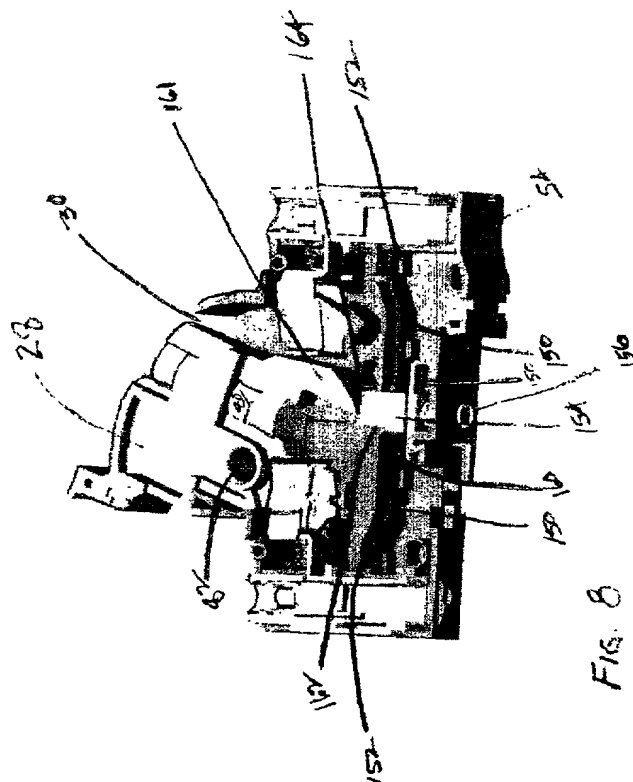


Fig. 8